



D.med healthcare

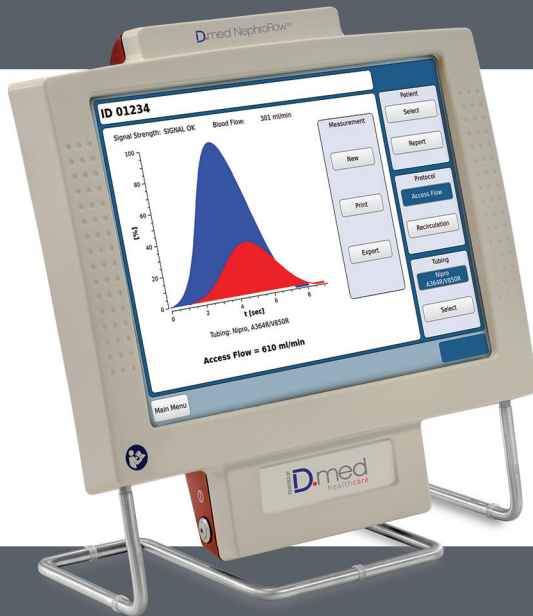

D.med
healthcare

Nephroflow™

- Clear 15" Touch screen
- Fast start and "Quick mode"
- Patient Database
- Highly accurate measurement
- Print and save via USB
- Separate stand, basket, plate and cover available
- Exchangeable Li-Ion battery pack

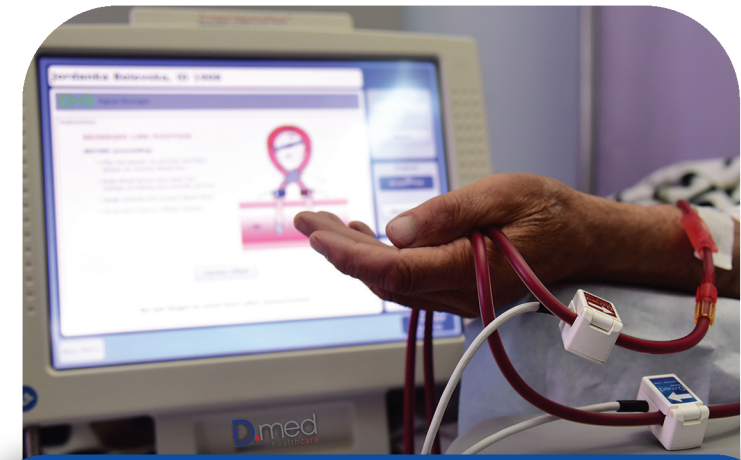

Recirculation and access flow measuring device

Vascular dialysis access is considered to be the Achilles heel of hemodialysis.

Based on the advice of the NKF KDOQI™, a monthly observation to diagnose and prevent stenosis or thrombosis progression is recommended.*

D.med NephroFlow enables this monitoring to take place using ultrasound dilution technology and non-invasive access flow monitoring. Safe, quick and accurate, the device provides the actual blood flow, access recirculation and shunt flow for your patient during hemodialysis.

The annual functional inspection can easily be done on site, without the need to remove the device from its operating environment. Furthermore, our tubing database is constantly updated and can easily be downloaded when needed.

*National Kidney Foundation: KDOQI clinical practice guidelines for vascular access
Updated 2006



LARGE TOUCH SCREEN

The highly sensitive screen optimizes usability during the treatment. An intuitive interface guides the user through measurement and provides all steps and necessary advice.



QUICK MEASUREMENT MODE

The quick mode allows the user to perform a measurement without entering patient data. D.med NephroFlow is ready to measure within seconds.



BUILT-IN FAST START

It takes only a few seconds to be ready to measure once the device is switched on. No lost time. Immediate effectiveness.





TREND VIEWER

Graphical documentation of previous measurements allows to supervise the vascular access of the patient and helps for proactive minimal intervention.



PRINT & SAVE VIA USB

In normal mode, all the data is immediately stored in the patient record. A simple USB connection allows you to export and/or print the data without needing an external PC.

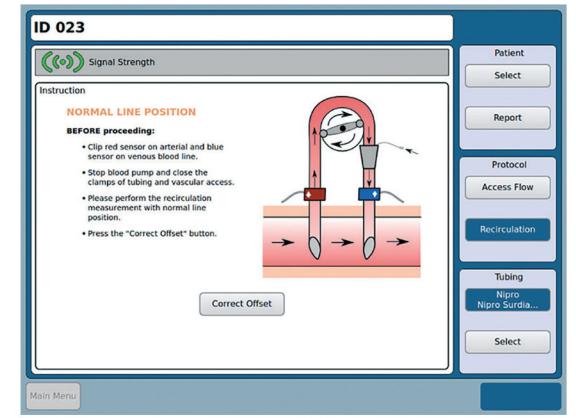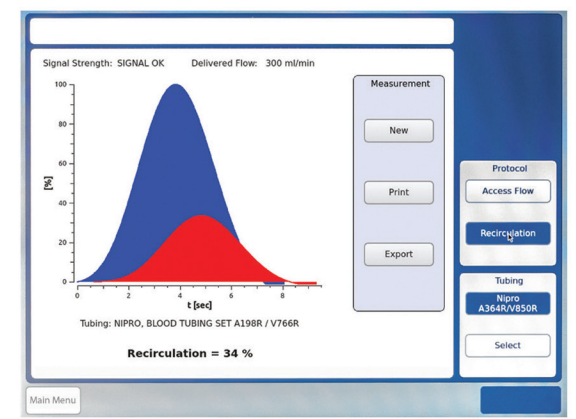

Products are continuously under review in the light of technical advancement; the actual specifications may therefore be subject to improvement or modification without notice. Some features and/or accessories displayed and described could be optional in different markets. The information provided does not constitute an offer to sell and is provided merely for informational purposes. Images published in the present document are shown exclusively for demo purposes, are representative for the possible applications and might be adapted for graphic needs. All rights reserved.

BIBLIOGRAPHY

References for Delivered Blood Flow:

Depner TA et al., "Pressure Effects on Roller Pump Blood Flow during Hemodialysis," ASAIO Transactions 1990; 36(3): M456-M459.

Sands JJ et al., "Difference between Delivered and Prescribed Blood Flow (QB) in Hemodialysis," ASAIO J 1996; 42(5): M717-M719.

References for Access Monitoring:

European Renal Association-European Dialysis and Transplant Association (ERA-EDTA). European Best Practice Guidelines on Hemodialysis Guideline 5.2 Nephrol Dial Transplant 2007; 22(Suppl 2): ii99-ii100.

National Kidney Foundation, NKF-K/KDOQI Clinical Practice Guidelines for Vascular Access: update 2006 Am J Kidney Dis 2006; 48 (Suppl1) 5176-276.

McCarley P et al., "Vascular Access Blood Flow Monitoring Reduces Access Morbidity and Costs," Kidney Int 2001; 60(3): 1164-1172.

References for Recirculation:

MacDonald J et al., "Identifying A New Reality: Zero Vascular Access Recirculation Using Ultrasound Dilution," ANNA J 1996; 23(6): 603-608.

Alloatti S et al., "Measurement of Vascular Access Recirculation Unaffected by Cardiopulmonary Recirculation: Evaluation of an Ultrasound Method," Nephron 1999; 81(1) 25-30.

Personally & Professionally
WE SERVE

We
Care

Contact

D.Med Healthcare GmbH & Co. KG
Klaus-Bungert-Str. 3, D-40468 Düsseldorf
phone +49 211 65 04 15 60
fax +49 211 65 04 15 61

dmednephroflow@dmed-healthcare.com
www.dmed-healthcare.com